

#### Accessories

- Device with 4 cables
- Self-adhesive electrodes
- Order form, patient diary and instructions
- Red closure clip for return

#### Return


Please return the device, order form and patient diary to us at the end of the recording. Viollier will cover the shipping costs.

- By customer service – delivery in practice
- By DPD – drop off at a pickup parcelshop → [dpdgroup.com/ch/mydpd/parcel-shops](http://dpdgroup.com/ch/mydpd/parcel-shops)
- By mail

Please note the following instructions for the return of the box:

- Remove label from window
- Slide the corresponding returns label (in the case) into the field of vision  
→ **Viollier AG address becomes visible**
- Close case with red closure clip

# IN STRUCTION

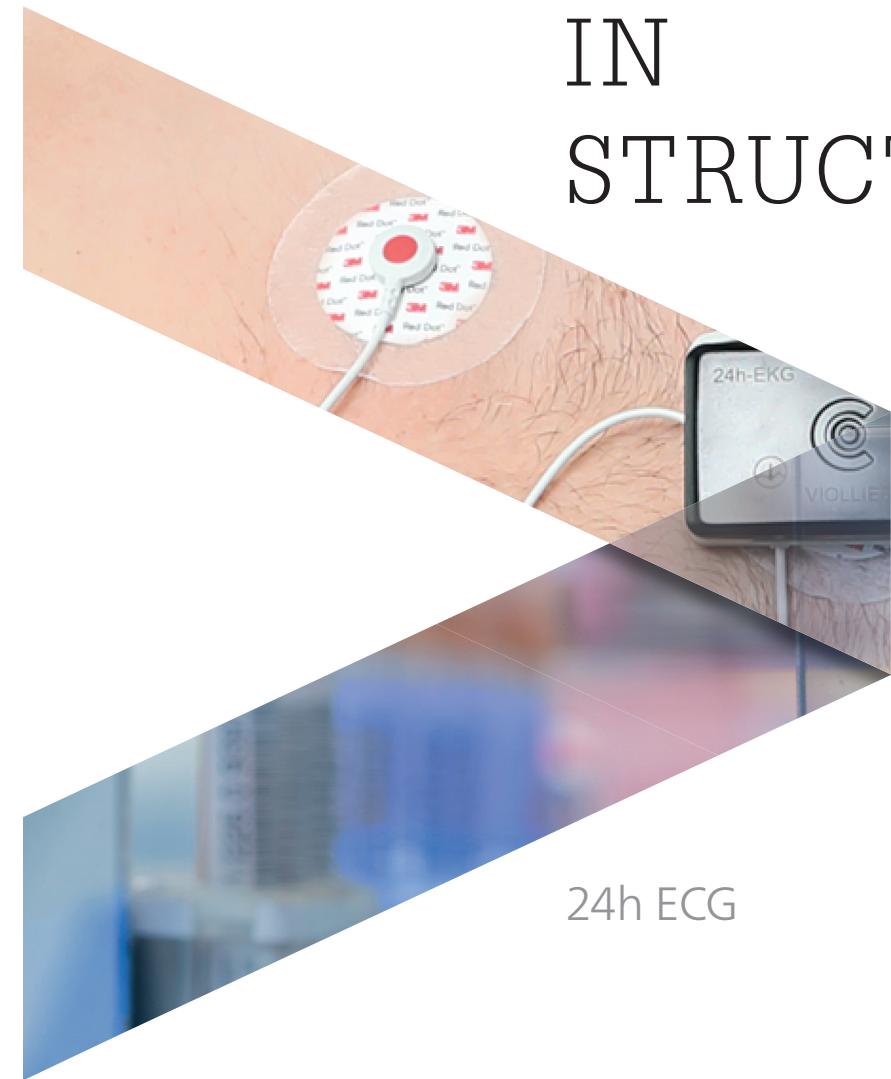

24h ECG

# Important information

Recording begins within 60 seconds of the electrodes making contact with the skin.

- Suitable for patients weighing 10 kg and over
- Do not use in the vicinity of CT, MRI and X-rays
- Mobile phones, strong electromagnetic sources and electric blankets can affect the quality of the recording.
- Wearing in the swimming pool, sauna, bathtub, shower or similar wet rooms is prohibited.



## Patient diary

Please inform the patient about the diagnostic importance of keeping a correct and complete patient diary.

- Please use a black ballpoint pen.
- Note start and end of recording with date and time.
- Enter date and time of symptoms, unusual activities, medicines and sleeping periods.

## Identification and analysis

- Patient's personal details
- The date you entered and the exact start time of the recording
- The monitor number entered by Viollier on the order form

Geräte-Nr.	006	Manschett-Nr.	
Chip-Nr.		Akku-Nr.	


Please use the enclosed order form only, as this already has your address on it.

# Attaching the monitor

## Preparation


- Degrease the skin using ethanol 70% and shave the hair for optimal adhesion of the electrodes.
- Attach the electrodes to the cable ends.
- Attach a disposable adhesive electrode to the push-button contact on the back of the device. **Please do not use any additional plaster or adhesive tape.**

The electrode is used to fix the device to the patient's chest. This reduces motion artifacts and improves the quality of the recording. This electrode has no medical / diagnostic function.

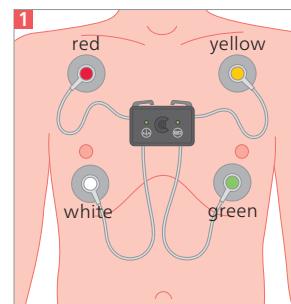

## Monitor mount

- Position the self-adhesive electrodes on the patient's chest as shown on image 1:
- red ● yellow ○ green ○ white
- Press the edge of the electrode firmly against the skin to fix it in place.
- The device starts automatically within 60 seconds of the electrodes making contact with the skin.

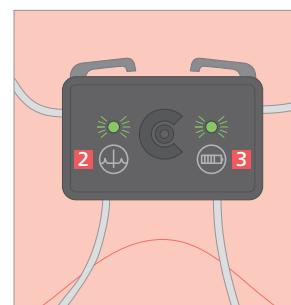

## Check recording mode

- The 'QRS complex' symbol 2 indicates the recording status.  
**Green flashing light:** ECG recording active
- The 'Battery' symbol 3 provides information on the charging status.  
**Green flashing light:** battery voltage sufficient

By tapping the device firmly with the flat of the hand, the patient can set a marker in case of discomfort.