


Instructions

7-day ECG

Patient diary

Please inform the patient about the diagnostic importance of filling out the patient diary correctly and completely.

- Please use a black ballpoint pen, not a pencil
- Note start and end of recording with date and time
- Enter date and time of symptoms, unusual activities, medicines and sleeping period

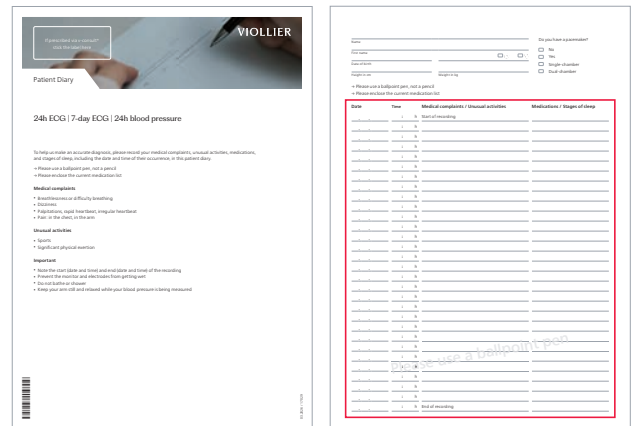

Identification and analysis

- Patient's personal details
- The date and exact start time of the recording, entered by you
- The monitor, cuff and chip card numbers entered by Viollier on the order form

Geräte-Nr.	006	Manschetten-Nr.	
Chip-Nr.	659	Akku-Nr.	010

Please only use the enclosed order form, as this already has your address on it

- If prescribed via v-consult®: print labels and stick them on all documents

Return

After completing the recording, please return the monitor with the battery plugged in (chip card in the monitor), order form and Patient diary. Viollier will cover the shipping costs.

- By customer service – return to practice
- By DPD – drop off at a pickup parcelshop → dpgdgroup.com/ch/mydpd/parcel-shops
- By mail


Please note the following instructions for the return of the box:

- Remove label from window
- Slide the appropriate return label (in the case) into the window → **Viollier AG address is visible**
- Close case with red clip

Important information

- **Connect the monitor and battery only when attached to the patient. The recording starts as soon as the monitor and the battery are connected**
- After completing the recording, return the monitor assembled
- Suitable for patients weighing 10 kg and over
- Do not use in the vicinity of CT, MRI and X-rays
- Mobile phones, strong electromagnetic sources and electric blankets can affect the quality of the recording

Attaching the monitor

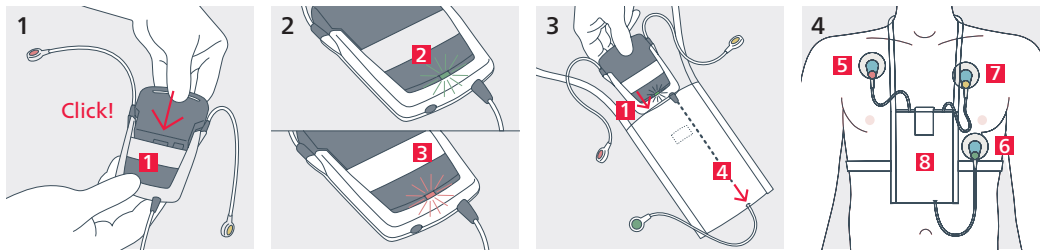

► VIOLLIER

1 Mounting the monitor

- Degrease the skin using ethanol 70% and shave the hair for optimal adhesion of the electrodes
- Push monitor and battery firmly together, connection clicks audibly

2

- Below the event button **1** a short fast flashing **green light 2** appear, followed by a **red light 3** and a slow flashing **green light 2**. The monitor is ready for the recording

3

- Pull the green cable through the small hole at the lower end of the protective pouch **4** and slide in the monitor
- Pull the neck strap and the monitor over the head → **dark grey event button 1 must be facing forward**

4

- Attach the self-adhesive electrodes as depicted in the diagram
- Attach the cable with the correct colors: **5** ● red, **6** ● green, **7** ● yellow
- If the patient wants to bathe or shower, the electrodes must be removed
- Change electrodes daily. New electrodes may be attached slightly offset to prevent redness

Recording

- The patient can trigger a new marking by himself
- In the event of symptoms this can be triggered by pressing the dark grey event button **1**.
If no symptoms are noticeable, the event ECG is able to recognize and record rhythm disorders by itself

Check recording mode

- **Green light:** recording in progress
- **Red light:** recording ended, dismount monitor and return
- Wear the monitor **8** in the protective pouch with a strap around the neck and fix it around the chest



Accessories

- Monitor with 3 cables and plugged-in chip card
- Battery
- Protective pouch with adjustable neck strap
- Self-adhesive electrodes
- Order form, Patient record and user guide
- Red closure clip for the return